

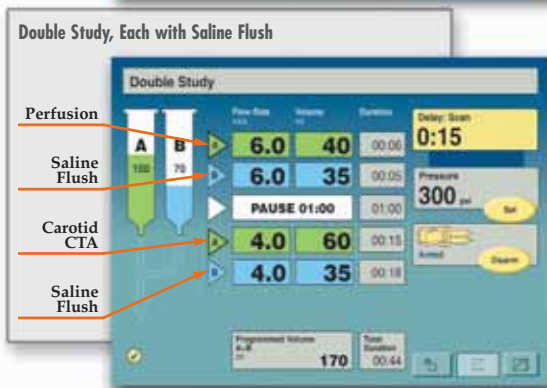


A Dedicated Dual-Head CT Injection System

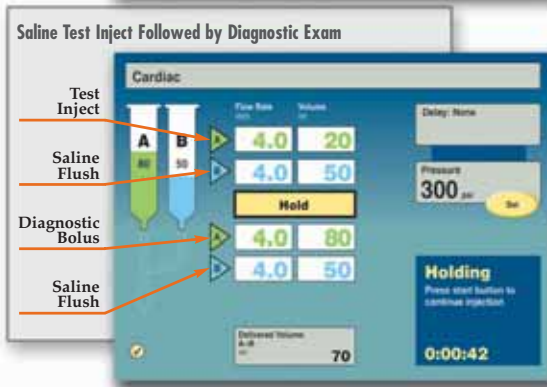

MEDRAD CT

"And as I've said, some studies just cannot occur unless you use a saline flush..."

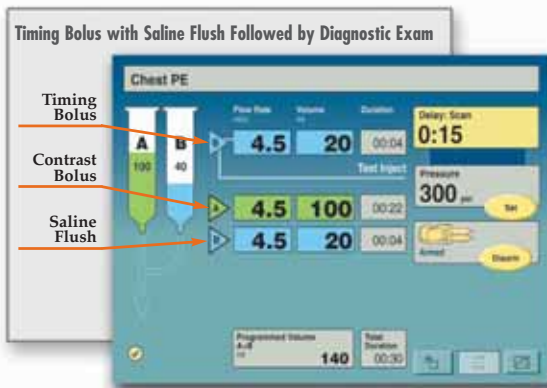

The MEDRAD Dual Difference

- Saline before and after CM*
- Hold/pause phase*
- Flexible programming*
- Simultaneous injection
- Imaging system interface (ISI)

* MEDRAD Patent US6339718 Programmable Injection Control

